


Aka-Brief #6 Coated Sintered Carbides

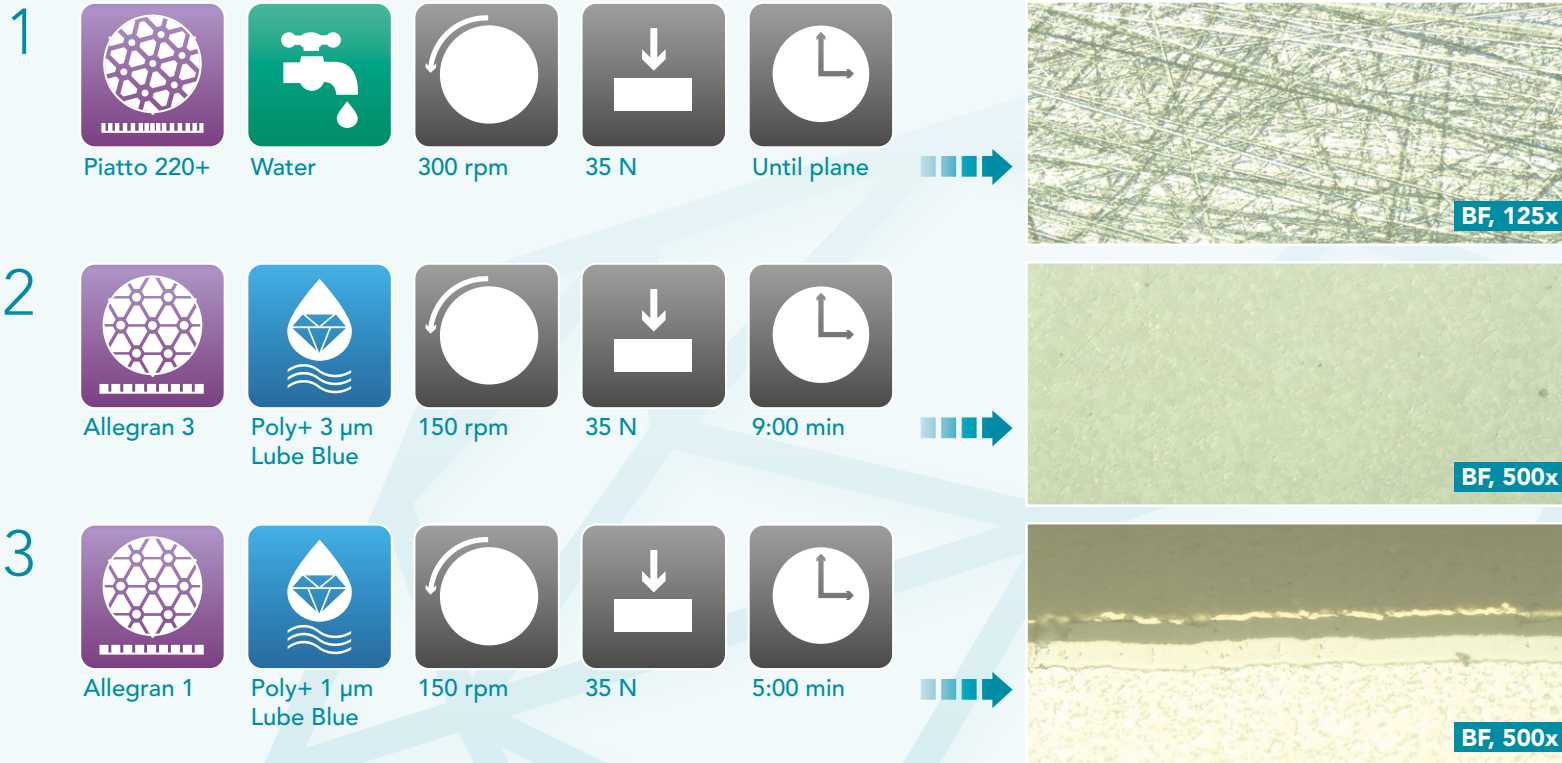

Times are stated for a 300 mm preparation system and Forces for an individual 40 mm dia. sample.

On a 250 mm system the times should be increased by 30%, on a 200 mm system by 100%.

With larger samples the force should be increased, with smaller samples decreased.

Time and Force may vary depending on the equipment.